

## GCX Mounting Assembly Operation/Installation Manual Dräger Model Julian-Plus® with Siemens SC9000 Patient Monitor with CPS



**Patient Monitor – Top Shelf / Power Supply on Right Side**

The purpose of these instructions is to:

1. Describe attachment of GCX mounting hardware to the Julian anesthesia machine.
2. Describe attachment of the Siemens monitor to the GCX mounting hardware.



**WARNING:** USE OF MOUNTING HARDWARE AND MONITORING COMPONENTS OTHER THAN THOSE DESCRIBED IN THIS DOCUMENT MAY RESULT IN SERIOUS INJURY DUE TO TIPPING OF THE ANESTHESIA MACHINE. ALL JULIAN MOUNTING CONFIGURATIONS REQUIRE THE COUNTERWEIGHT “BIGFOOT” UPGRADE SET AVAILABLE FROM DRÄGER.



Dräger P/N	Description
8601798	Julian Extended Base “Bigfoot” for new devices
8601824	Julian Extended Base “Bigfoot” for retrofits

*Installer: When installation is completed, provide these instructions to the end user for future reference.*

### INSTALLATION

#### **Option 1 – SC9000 on Top using Low Profile Horizontal Mount & Power Supply on Right Side**


Tools Required: Philips head screw driver

#### **Attach Julian Top Shelf Base Plate**

- 1) Install according to the instructions included with the Top Shelf Base Plate.


#### **Install Horizontal Channel Mount into Channel**

- 1) Align the Slide of the mount with edge of the Horizontal Channel insert into channel. Tighten the (2) #8-32 x 7/16” PHMS to secure position of the mount in the channel.

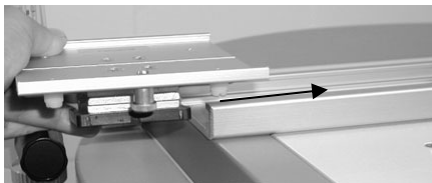

### Slide Pick & Go Base into Mounting Plate

- 1) Align the mounting adapter located at the bottom of the Pick & Go base with the edge of Mounting Plate. Slide the Pick & Go base into the plate until it stops at the Spring Plunger (located below the Mounting Plate). Pull the Spring Plunger and continue to slide the base until the mounting adapter engages the Spring Plunger.

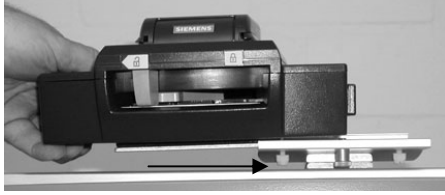

### Install 4" Julian Channel



- 1) Install according to the instructions included with the Channel.

### Install Power Supply Mounting Adapter to Siemens Power Supply Mount (Siemens P/N: 4720129)

- 1) Install according to the instructions included with the adapter.

### Slide Power Supply Mount into Channel & Insert Power Supply

- 1) Align the Slide of the mount with edge of the Channel insert into channel.

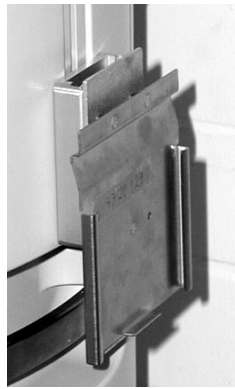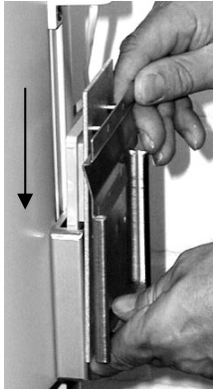

### Option 2 – SC9000 on Top using Low Profile Tilt Swivel Mount & Power Supply on Right Side


Tools Required: Philips head screw driver, Hex key (incl.).

#### Attach Julian Top Shelf Base Plate

- 1) Install according to the instructions included with the Top Shelf Base Plate.


#### Install Low Profile Tilt Swivel Mount into Channel

- 1) Align the Slide of the mount with edge of the Horizontal Channel insert into channel. Tighten the (2) 8-32 x 7/16" PHMS to secure position of the mount in the channel.

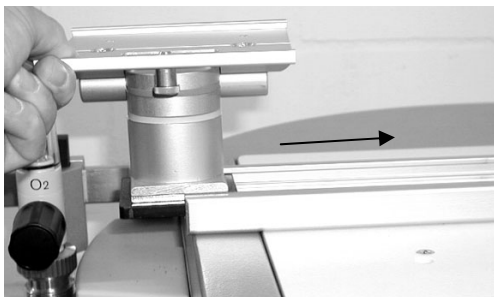

### Slide Pick & Go Base into Mounting Plate

- 1) Align the mounting adapter located at the bottom of the Pick & Go base with the edge of Mounting Plate. Slide the Pick & Go base into the plate until it stops at the Spring Plunger (located below the Mounting Plate). Pull the Spring Plunger and continue to slide the base until the mounting adapter engages the Spring Plunger.

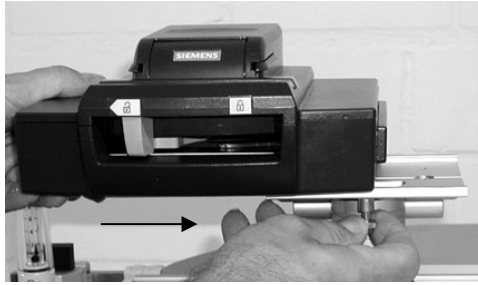

### Install 4" Julian Channel


- 1) Install according to the instructions included with the Channel.

### Install Power Supply Mounting Adapter to Siemens Power Supply Mount (Siemens P/N: 4720129)

- 1) Install according to the instructions included with the adapter.

### Slide Power Supply Mount into Channel & Insert Power Supply

- 1) Align the Slide of the mount with edge of the Channel insert into channel.

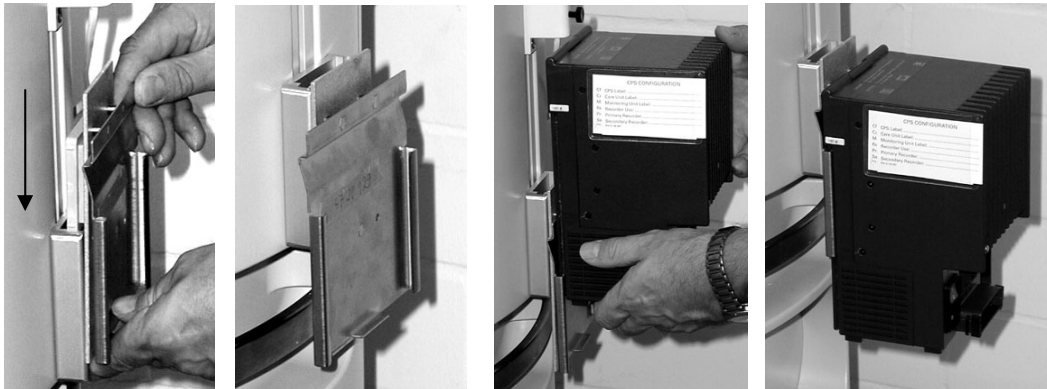

## Cleaning

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone and trichloroethylene.
3. Steel wool or other abrasive material should never be used.
4. Damage caused by the use of unapproved substances or processes will not be warranted. To verify compatibility, it is recommended that any cleaning solution be tested on a small area of the arm that is not visible.
5. Never submerge the mounting arm. Wipe any cleaning agents off of the arm immediately, using a water-dampened cloth. Dry the arm thoroughly after cleaning.

**CAUTION:** GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions supplied with those products.

## PARTS LIST

### Option 1

GCX P/N	Dräger P/N	DESCRIPTION
DR-0015-87 or	MM15736	Julian Top Shelf Base Plate w/20" Horizontal Channel
DR-0015-88	MM15737	Julian Top Shelf Base Plate w/10" Horizontal Channel
HZ-0001-01	MM15738	Low Profile 10 Degree Horizontal Mount
HZ-0003-01	MM15741	Low Profile 0 Degree Horizontal Mount

### Option 2

GCX P/N	Dräger P/N	DESCRIPTION
DR-0015-87 or	MM15736	Julian Top Shelf Base Plate w/20" Horizontal Channel
DR-0015-88	MM15737	Julian Top Shelf Base Plate w/10" Horizontal Channel
HZ-0002-01	MM15693	Low Profile Tilt/Swivel Mount

### Power Supply (CPS)

GCX P/N	Siemens P/N	Dräger P/N	DESCRIPTION
	4720129		Siemens Power Supply Holster
SI-0041-06	--	MM15754	Flush Mount for Siemens P/N 4720129
DR-0016-82	--	MM15707	4" Channel w/ T-Nuts