
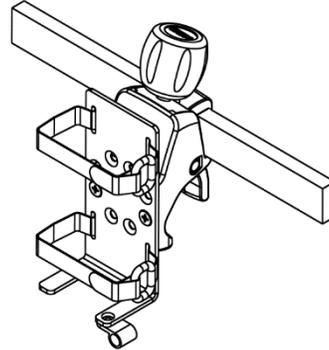



Installation Guide Power Supply Holster with PRC Post/Rail Clamp for .75" to 1.5" [19 mm - 38mm] Diameter Post or 10mm X 25mm Rail

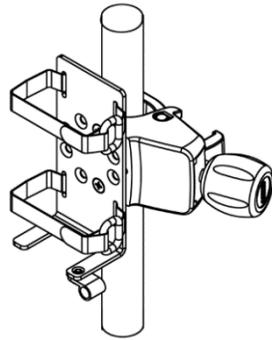

Parts Reference

The following parts and hardware are included with this kit (hardware not shown).

Item #	Description	Qty
1	Power Supply Holster with PRC Post/Rail Clamp	1
2	10-32 X 3/8" Flat Head Machine Screw	2
3	Plastic Cable Clamp	1
4	Flat Washer	1
5	8-32 X 1/4" Pan Head Machine Screw	1
6	18" Velcro Strap	2

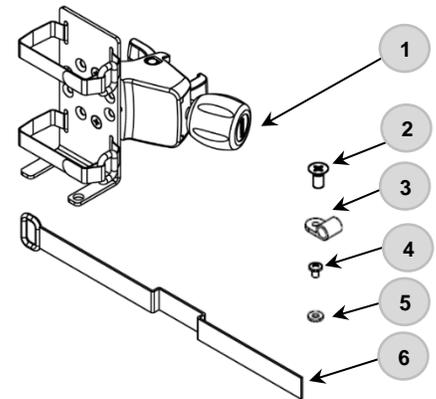


Tools Required:

Phillips Screwdriver (not supplied)





Warning - The maximum load rating for this product is 30 lbs. [13.6 Kg] at Clamp.

Mounting Power Supply on Post

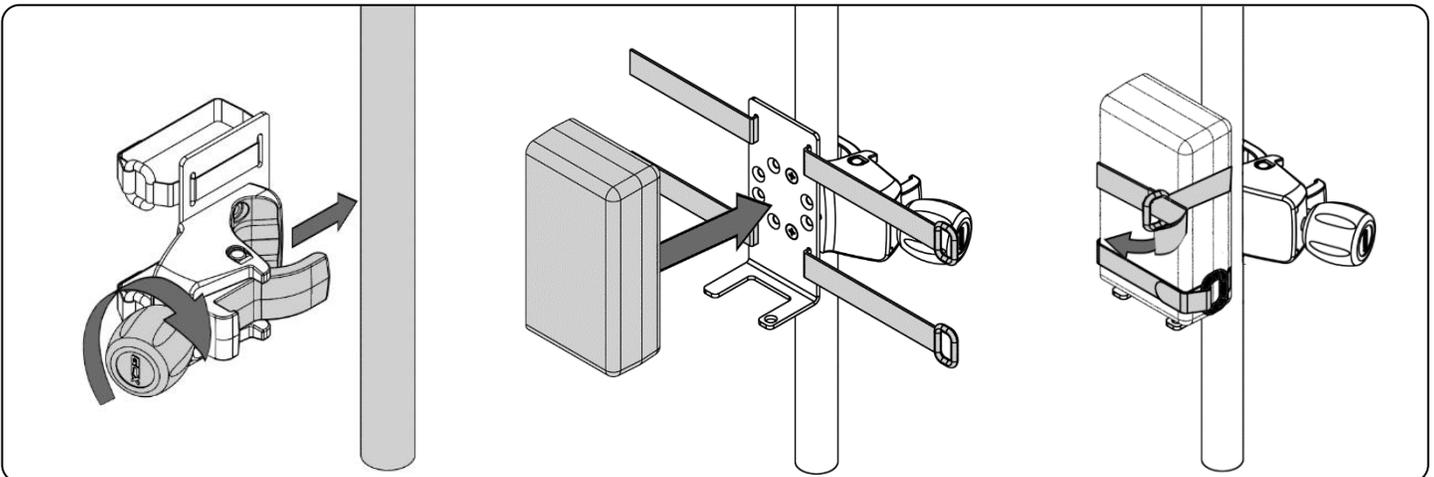


Open Clamp by turning knob counterclockwise (CCW). Position Clamp around post and turn Knob clockwise (CW) to tighten.

Mounting Power Supply to Rail

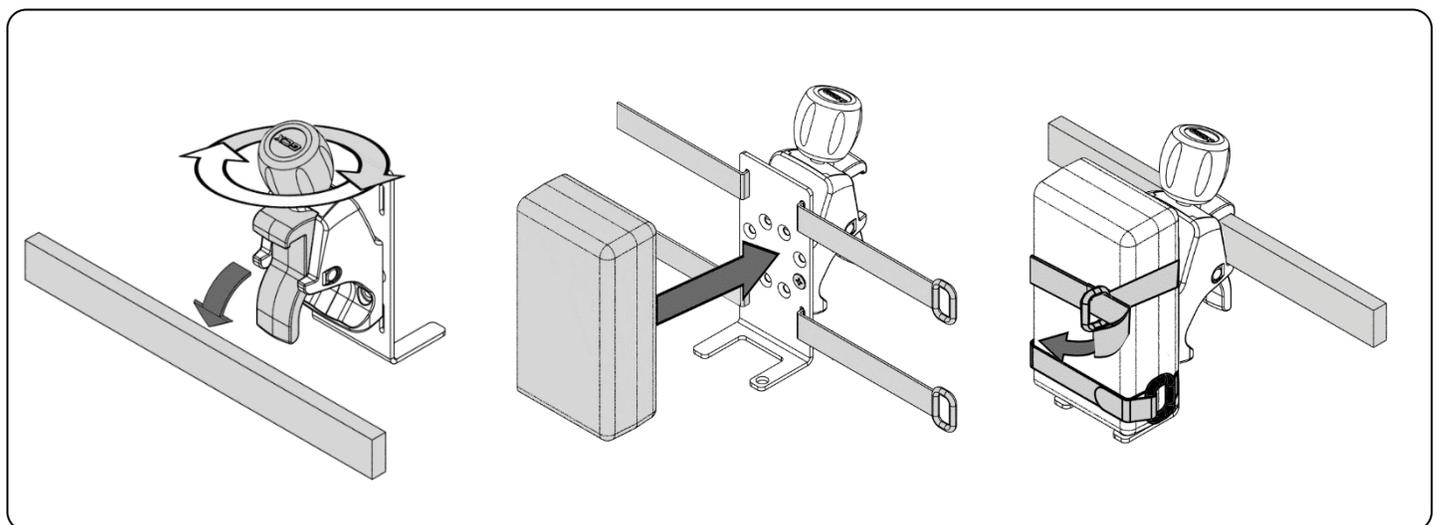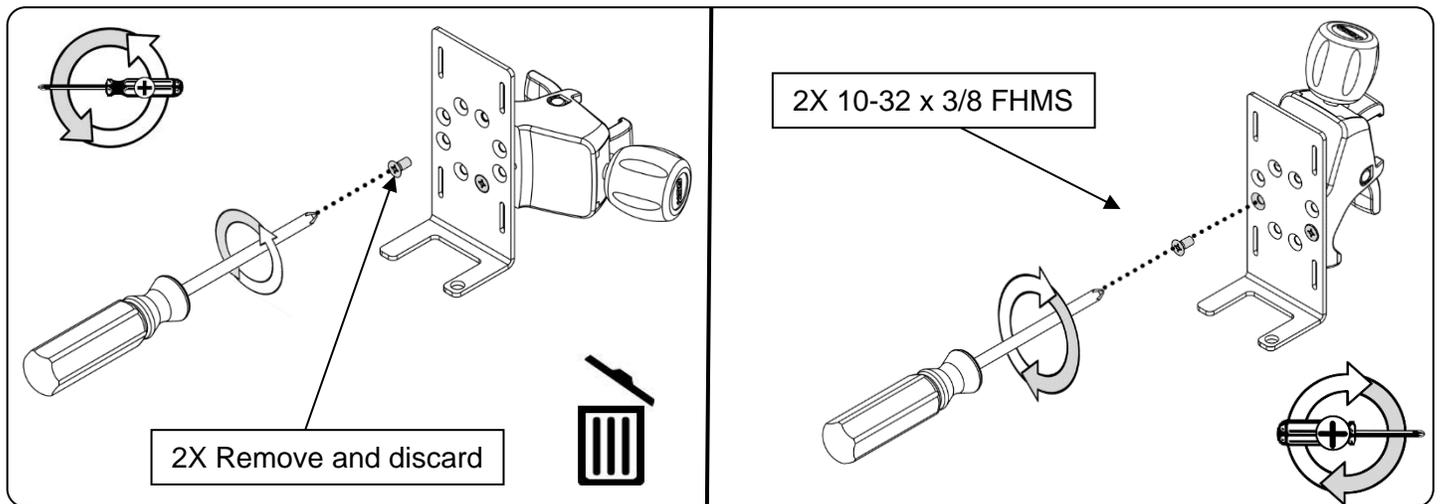

Open Clamp by turning knob counterclockwise (CCW). Position Clamp around Rail and turn Knob clockwise (CW) to tighten.

Cable Management

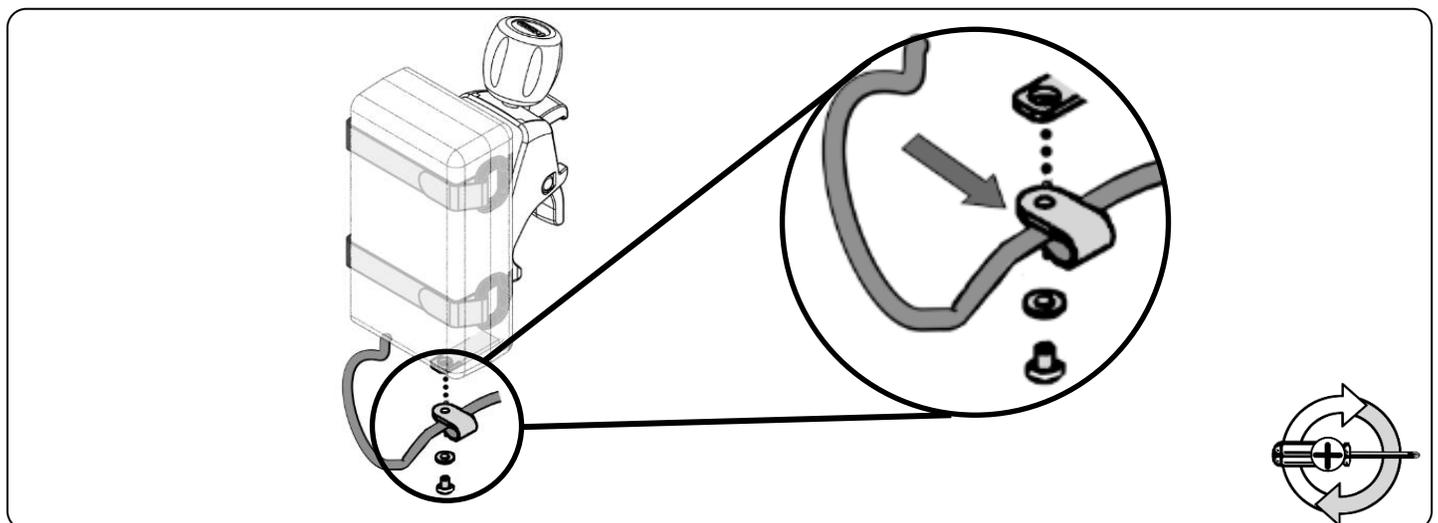



Routine Maintenance

Periodically inspect all fasteners associated with the mounting system. Tighten or adjust fasteners as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g., diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.
3. Do not use Steel wool or other abrasive material.
4. Damage caused using unapproved substances or processes will not be warranted. It is recommended that you test any cleaning solution on a small area of the arm that is not visible to verify compatibility.
5. Never submerge or allow liquids to enter the mounting assembly. Wipe any cleaning agents off of the arm immediately, using water dampened cloth. Dry the arm thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment refers to the specific instructions delivered with those products before installing the arm in the Channel.