


Installation Guide

Roll Stand Kit For Mortara Surveyor S12 Monitor


The purpose of this guide is to describe assembly of the Roll Stand.

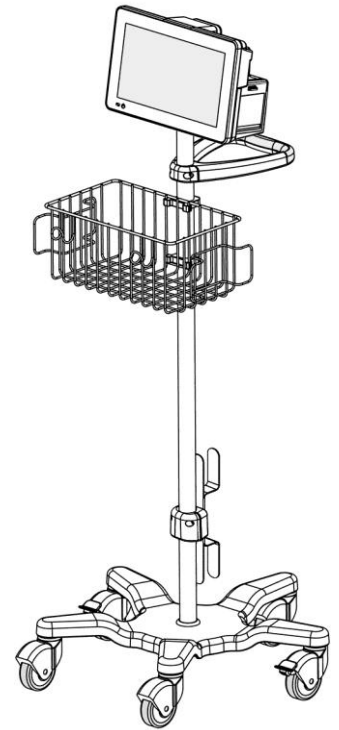

Parts Reference

The following parts and hardware are included with this installation kit (hardware not shown):

Item #	Description	Qty
1	40" Roll Stand Post	1
2	21" Roll Stand Base	1
3	Mounting Plate / Power Supply Holster	1
4	Quick Connect VESA Adapter	1
5	Handle (includes mounting hardware)	1
6	Utility Basket (includes mounting clips)	1
7	Cord Wrap (includes mounting hardware)	1
8	Tapered Plug	1
9	M4 x 16mm Button Head Cap Screw (BHSCS)	4
10	5/16-18 x 1 3/4" Hex Head Cap Screw (HHCS)	1
11	5/16 Flat Washer	1
12	5/16 Split Lock Washer	1
13	10-32 x 3/8 Flat Head Machine Screw (FHMS)	2
14	2.5mm Hex Wrench	1

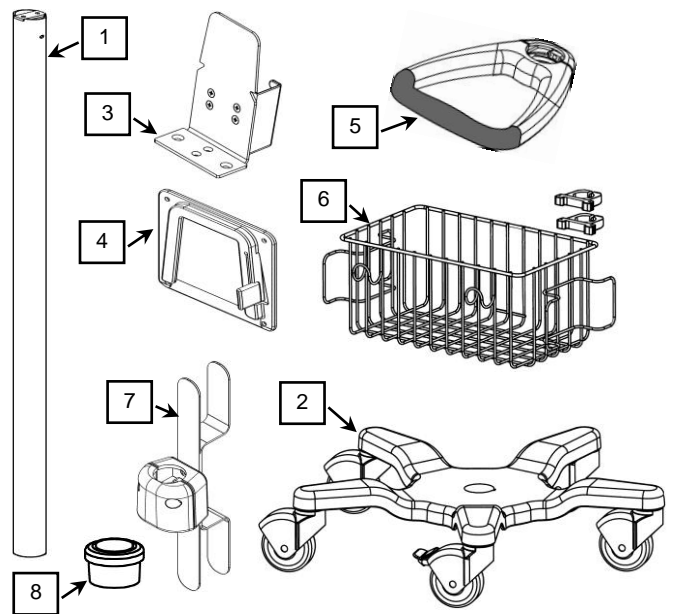


Tools Required

- Phillips screwdriver (not provided)
- 1/2" [13mm] wrench (not provided)
- 2.5 mm Hex Wrench (provided)

Attaching Roll Stand Post to Base



Installation Note: Roll stand post has (2) threaded mounting holes on top, and (1) threaded mounting hole on the bottom.

Slide the tapered plug onto the bottom of the roll stand post. Using a 1/2" [13 mm] socket wrench, fasten post to base with one (1) 5/16-18 x 1 3/4" HHCS, (1) 5/16 split lock washer, and (1) 5/16" flat washer as shown below.


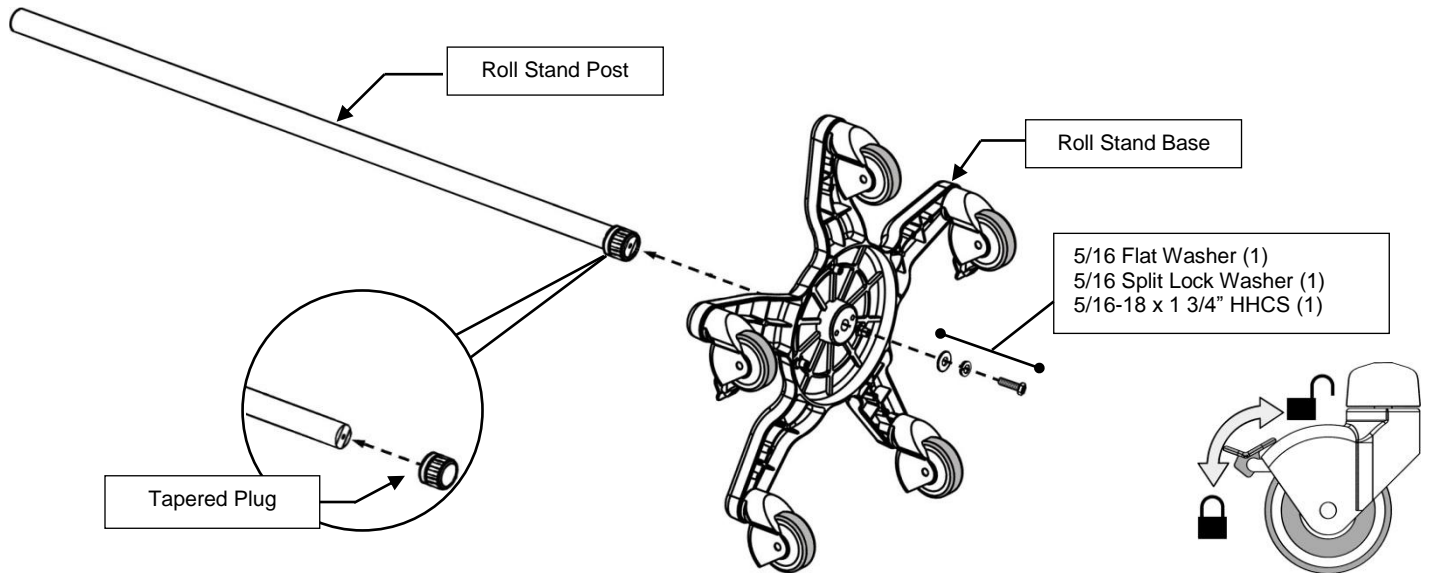


Installing Basket on Post

1. Install (2) nylon mounting clips at an angle in center of the basket and rotate until both are horizontal (Fig. A). Slide the mounting clips to the top and bottom of basket. The top clip should be touching the top horizontal wire, and the bottom clip should be touching the lower reinforcing wire (Fig. B).

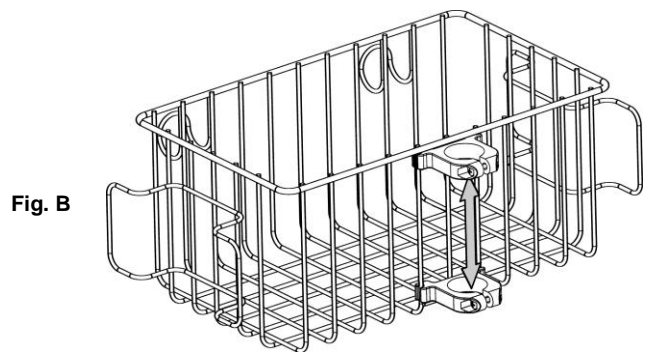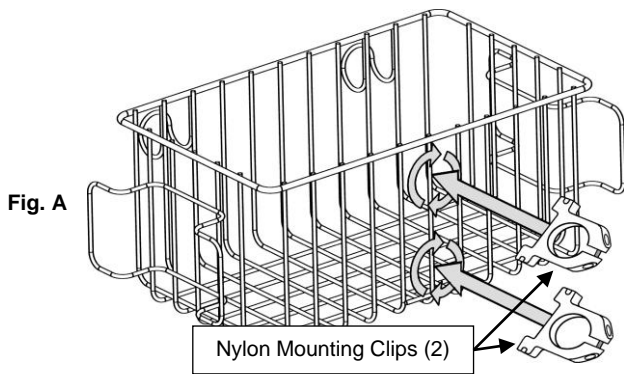


2. Slide Clips over the top end of the roll stand post and position basket at desired height (Fig. C). Using a Phillips screwdriver, alternately tighten the mounting clip screws until basket does not rotate on post (Fig. D).

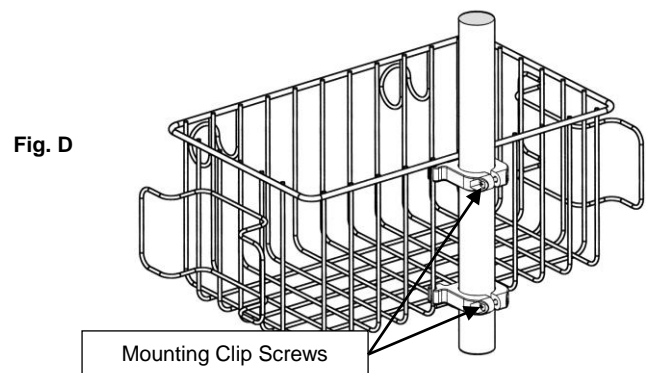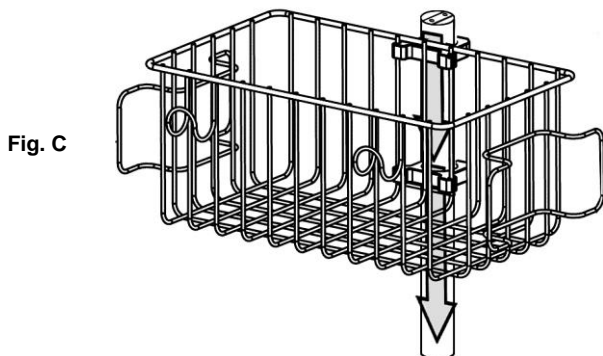


Attaching the Roll Stand Handle

Fasten Handle to Roll Stand Post with (2) #10-32 x 9/16" PHMS. Alternately tighten Handle screws until handle does not rotate around post.

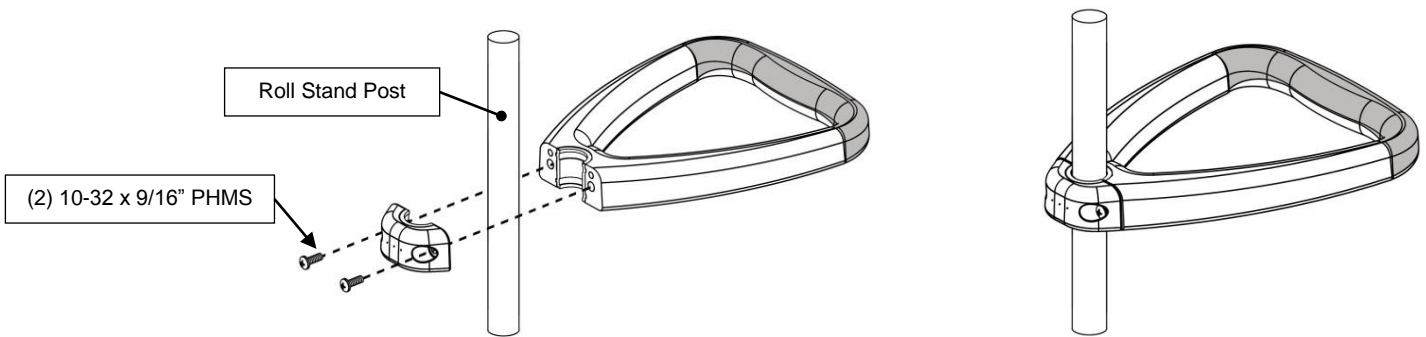


Attaching the Mounting Plate to Post

Using a Phillips screwdriver, attach the Mounting Plate to Roll Stand Post with (2) #10-32 x 3/8" FHMS as shown below.

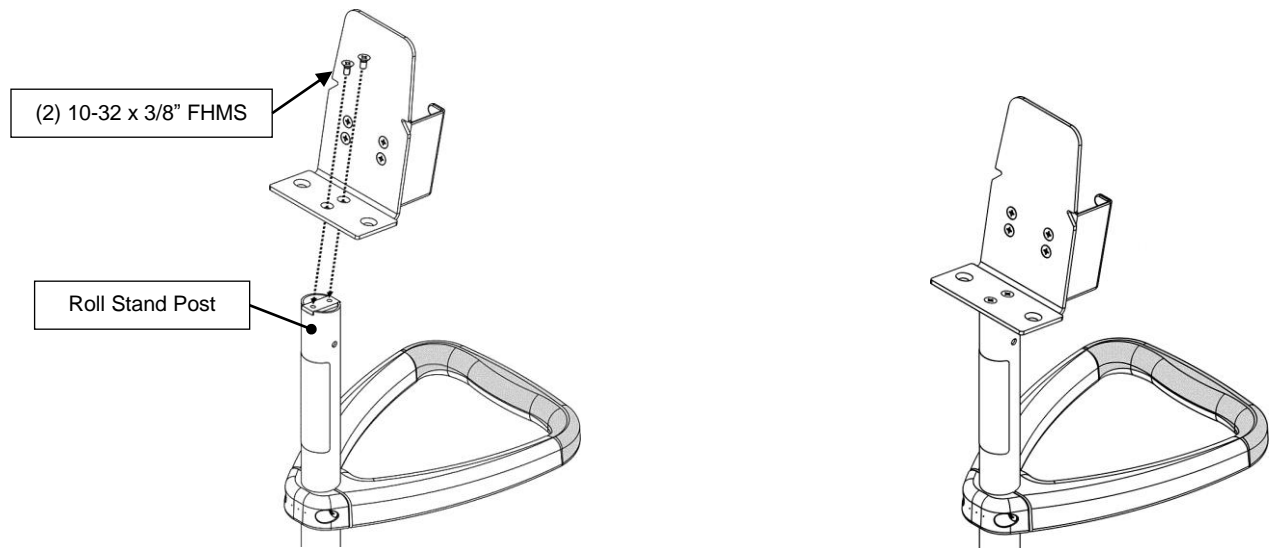


Attaching the Cord Wrap to Post

Using a Phillips screwdriver, attach the Cord Wrap to Roll Stand Post with (2) #10-32 x 9/16" PHMS. Alternately tighten screws until Cord Wrap is secure and does not rotate on post.

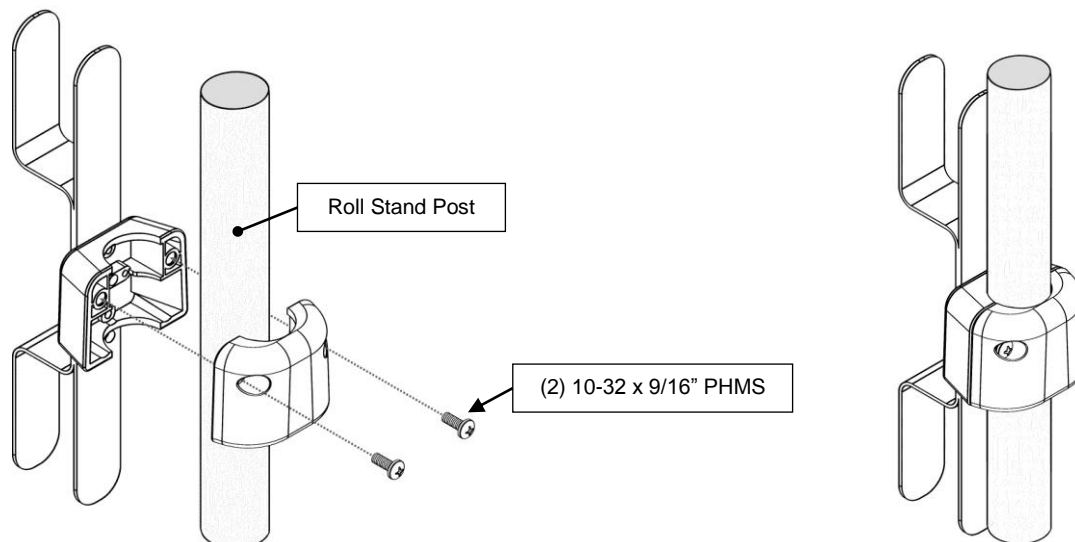


Installing the Quick Connect VESA Adapter

Using a 2.5mm hex wrench (provided), secure VESA Adapter to the monitor with (4) M4 x 16mm BHSCS.

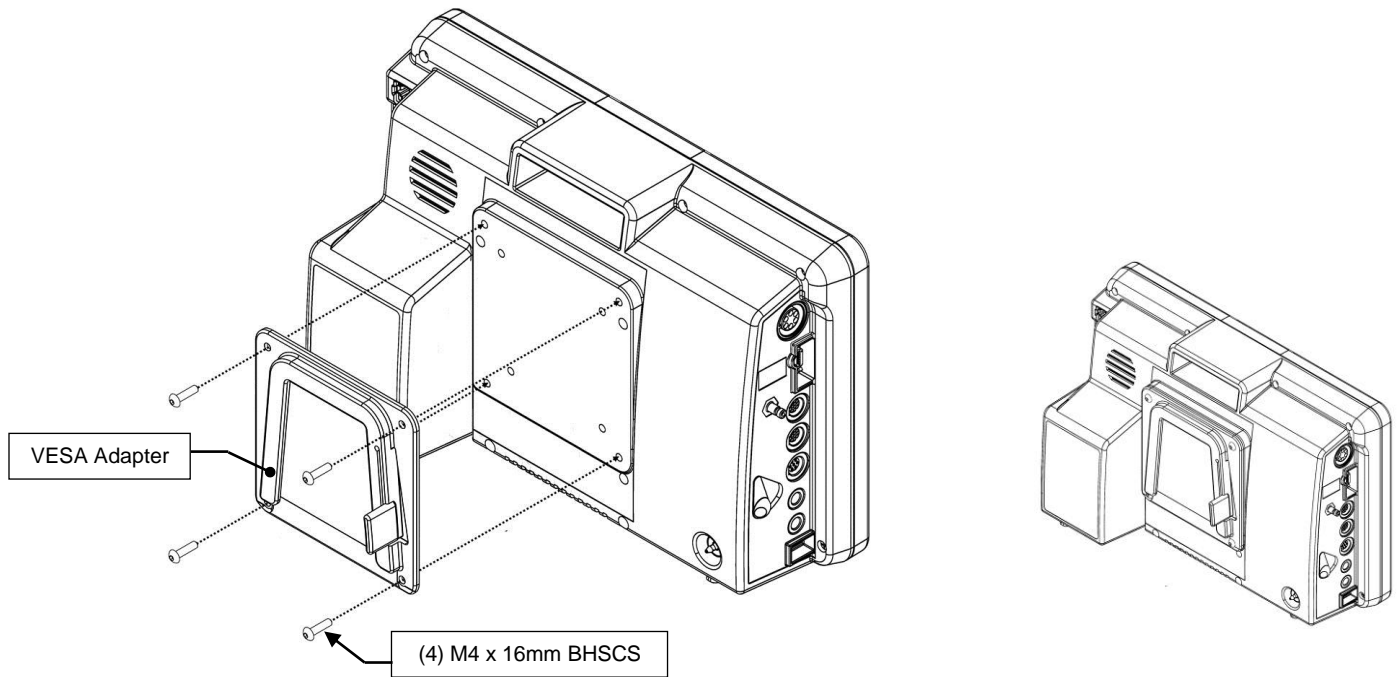

Installing the Monitor onto the Mounting Plate

Lower the monitor downward onto the mounting plate until the release lever on the VESA Adapter locks into place.

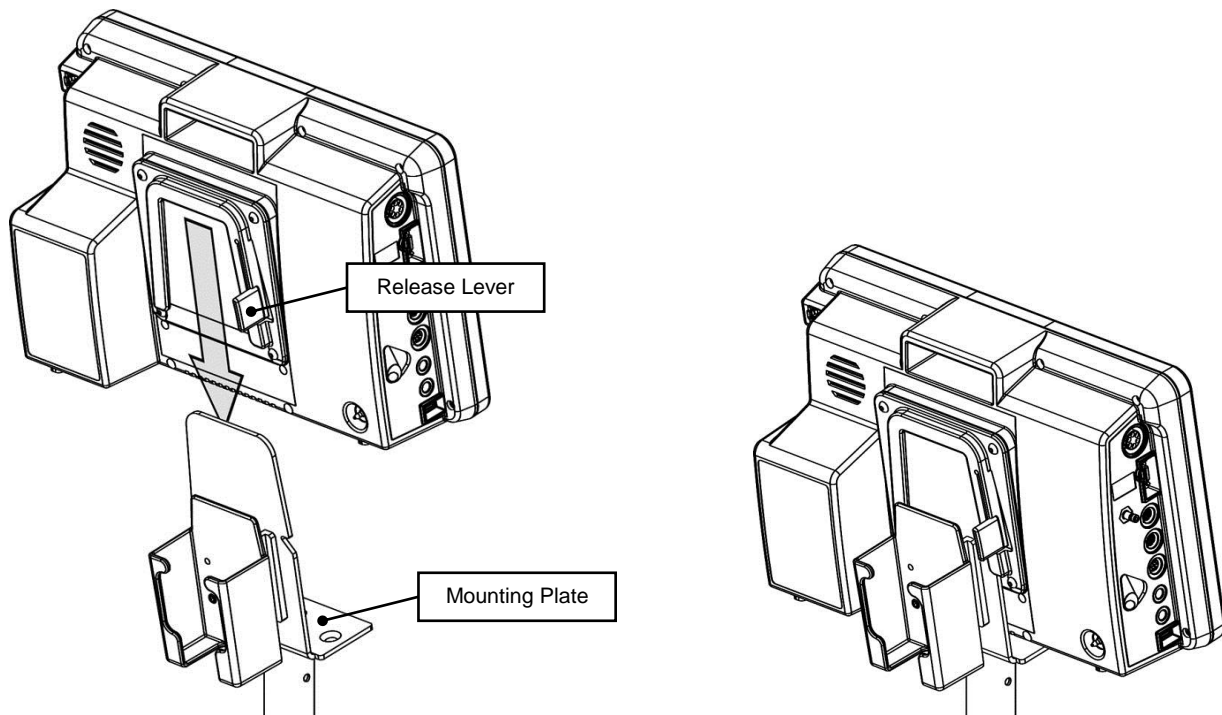

Routine Maintenance

Periodically inspect all fasteners associated with the mounting system. Tighten or adjust as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone and trichloroethylene.
3. Do not use steel wool or other abrasive material to clean the mounting assembly.
4. Damage caused by the use of unapproved substances or processes will not be covered by warranty. We recommend testing of any cleaning solution on a small area of the mounting assembly that is not visible to verify compatibility.
5. Never submerge the roll stand or allow liquids to enter the mounting assemblies. Wipe any cleaning agents off the mounting assembly immediately using a water-dampened cloth. Dry all mounting assemblies thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted instruments or accessory equipment, refer to the specific instructions delivered with those products.