

Installation Guide

16" [40.6 cm] Channel for Dual Rails 8 to 10 mm (W) x 25 to 30 mm (H)

The purpose of this guide is to describe mounting of Channel on rails (page 2).



WARNING: The customer must verify the stability of the rails on which the 16" Channel will be mounted. The maximum load rating of the Channel is 60 lbs [27.2 kg].


Parts Reference

The following parts are included with this installation kit:


Item #	Description	Qty
1	Channel Assembly	1
2	3/16" Hex Wrench	1

Tools Required


- 3/16" hex wrench (provided)
- Phillips screwdriver (not provided)

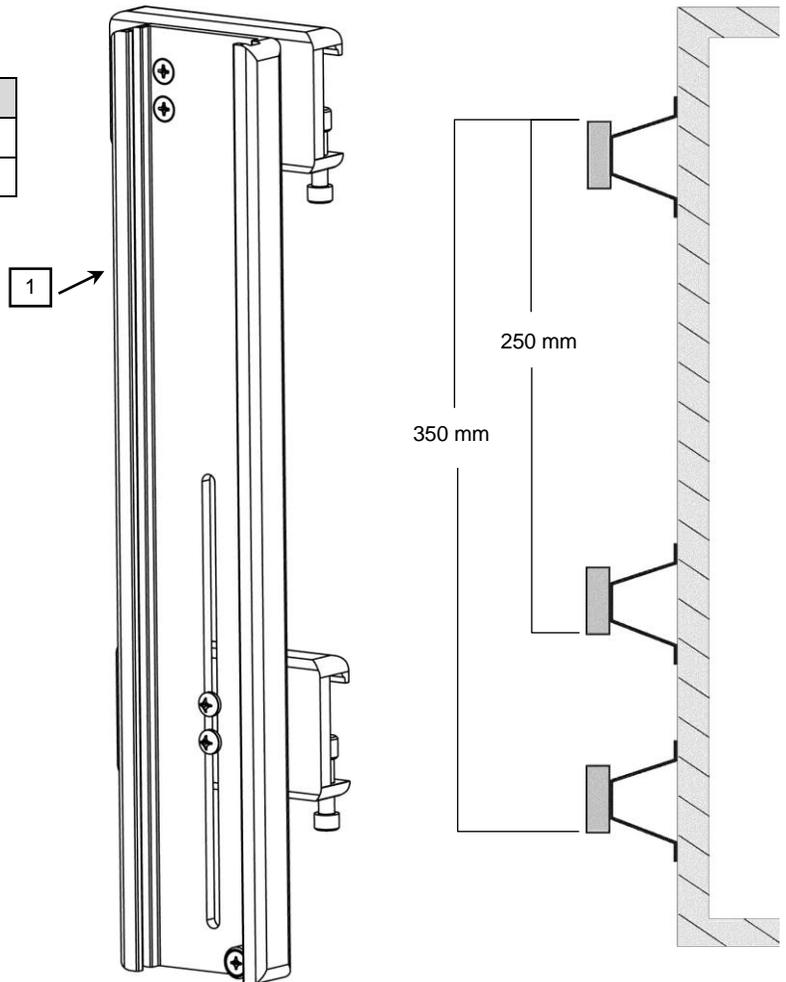

Mounting Channel on Rails

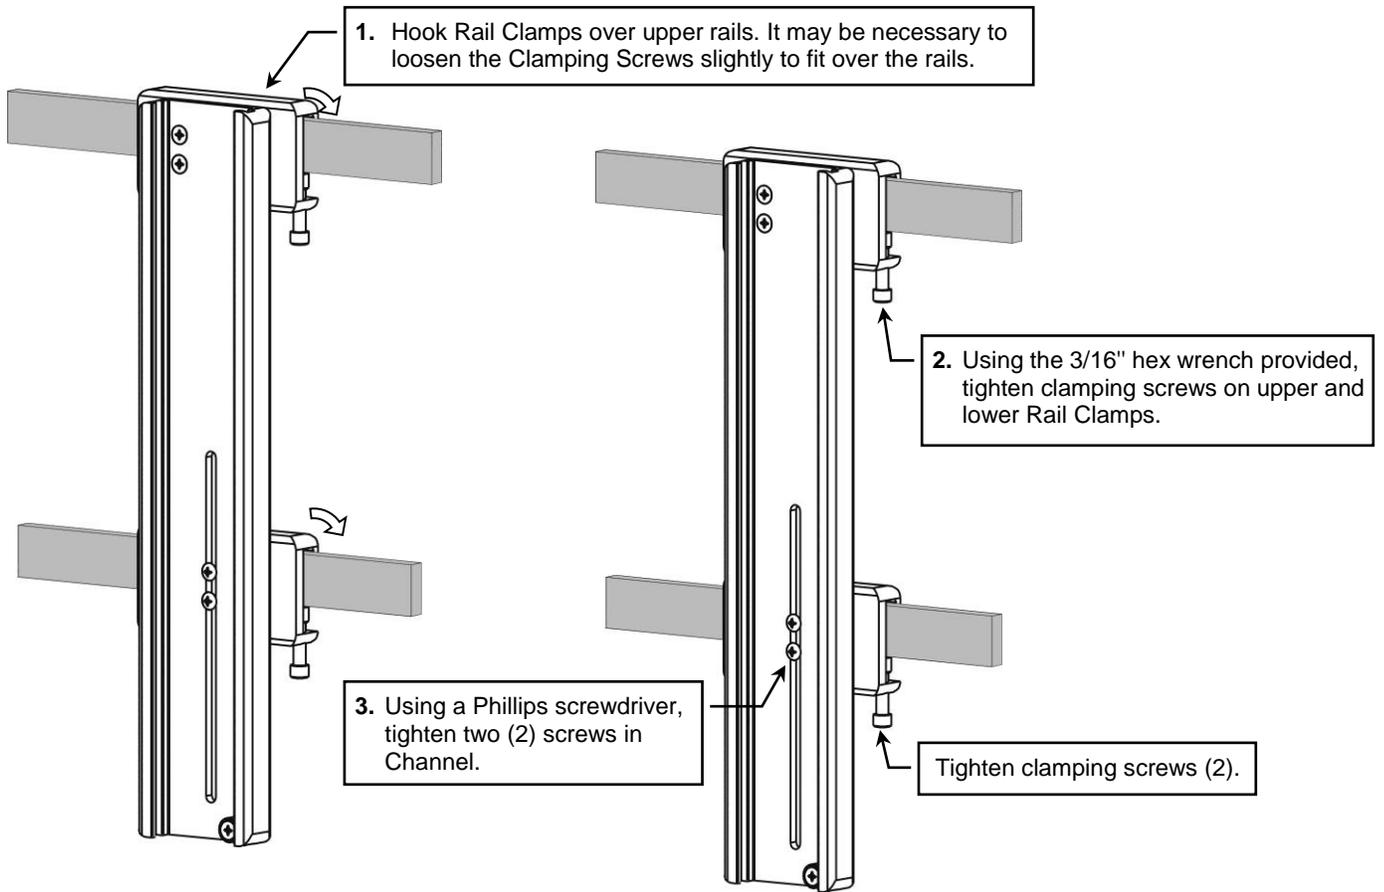

Moving the Lower Rail Clamp

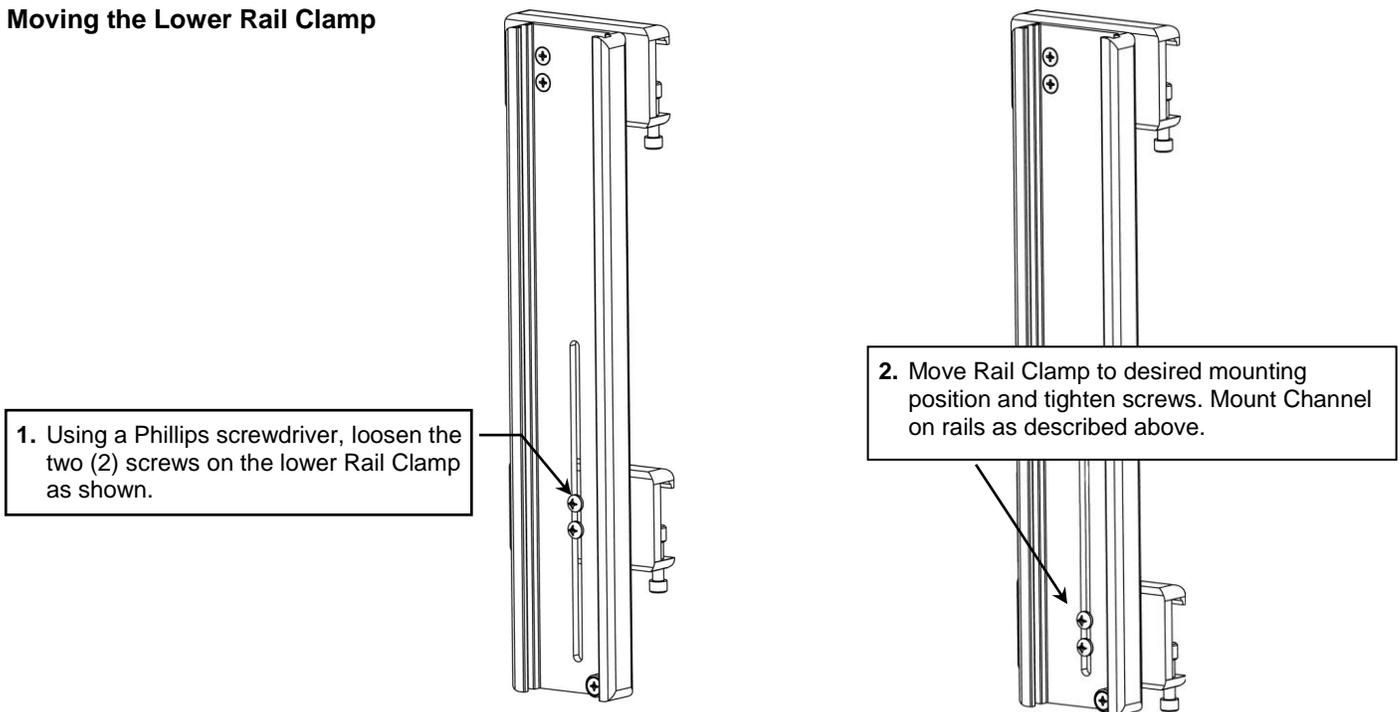

Routine Maintenance of the Mounting Assembly

Periodically inspect all mounting hardware. Tighten or adjust as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted instruments or accessory equipment, refer to the specific instructions delivered with those products.

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone and trichloroethylene.
3. Do not use steel wool or other abrasive material to clean the mounting assembly.
4. Damage caused by the use of unapproved substances or processes will not be covered by warranty. We recommend testing of any cleaning solution on a small area of the mounting assembly that is not visible to verify compatibility.
5. Never submerge or allow liquids to enter the mounting assembly. Wipe any cleaning agents off of the mounting assembly immediately using a water-dampened cloth. Dry mounting assembly thoroughly after cleaning.