

Installation Guide

Stor-Locx Adapter Kit-VHRS Applications

Parts Reference

The following parts and hardware are included in this adapter kit.

Item #	Description	Qty
1	Stor-Locx Adapter Bracket	1
2	1/4-20 x 1" Flat Head Socket Cap Screw (FHSCS)	4
3	10-32 x 5/8" Socket Head Cap Screw (SHCS)	3
4	5/32 Hex Wrench	1
5	Screw Head Covers (not shown)	4







Tools Required: 5/32 Hex Wrench (provided)

Attaching Adapter Bracket to VHRS

1. Using a 5/32" hex wrench, attach the Adapter Bracket to the top of the VHRS with (3) 10-32 x 5/8" SHCS.

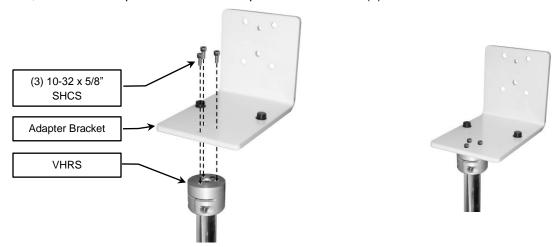


2. Remove and discard the (4) mounting screws and Channel Slide attached to the back of the Enclosure.

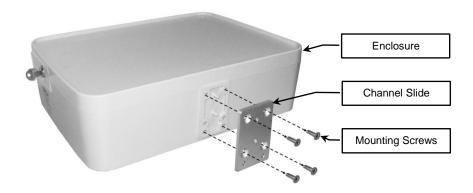

3. Align the (2) Guide Pins on the back of the Enclosure with the (2) corresponding Guide Pin holes on the Adapter Bracket as shown (below left). Using a 5/32" Hex Wrench, secure Enclosure to Adapter Bracket with (4) 1/4-20 x 1" FHSCS



4. Apply the (4) self-adhesive Screw Head Covers.

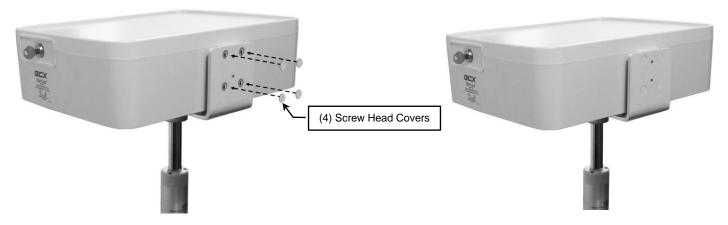

Periodic Maintenance

All fasteners associated with the mounting system should be inspected periodically and tightened as necessary.

Cleaning the Mounting Assembly

- 1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
- 2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.
- Steel wool or other abrasive material should never be used.
- 4. Damage caused by the use of unapproved substances or processes will not be warranted. It is recommended that you test any cleaning solution on a small area of the mounting assembly that is not visible to verify compatibility.
- 5. Never submerge or allow liquids to enter the mounting assembly. Wipe any cleaning agents off the assembly immediately, using a water dampened cloth. Dry the assembly thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions delivered with those products.